

Contents lists available at ScienceDirect

Brain Stimulation

journal homepage: http://www.journals.elsevier.com/brain-stimulation



Ramped V1 transcranial ultrasonic stimulation modulates but does not evoke visual evoked potentials



Transcranial ultrasonic stimulation (TUS) is an emerging non-invasive brain stimulation technique that has higher spatial resolution than electrical and magnetic stimulation approaches, and, uniquely, offers the ability to target structures deep in the brain. Early work in humans suggests that TUS can both evoke neural activity [1] and modulate activity elicited by other stimuli [2]. However, the protocols used in these studies may be audible due to the sharp onset and offset of ultrasound energy [3,4], and it is therefore possible that there is an auditory confound to the observed effects [5]. Here, therefore, we used a less audible, ramped protocol [3] to determine if we could either evoke or modulate activity in the primary visual cortex (V1).

We examined whether V1 TUS alone evokes neural activity detectable in the EEG, and whether TUS modulates visual evoked potentials (VEPs) in response to a pattern-reversal checkerboard stimulus. Fourteen healthy participants (4 female, 31 ± 4.3 years) were included in the study, after excluding three participants due to technical problems. The project was approved by the UCL research ethics committee (Project ID 14071/001).

As described in our previous paper [3], TUS was delivered using a 2-element spherically focusing annular array transducer (H115-2AA, Sonic Concepts) with a nominal outer aperture diameter and radius of curvature of 64mm. The transducer was driven at 270 kHz by a 2-channel TPO (Sonic Concepts) with the output power and element phase adjusted to give a focal pressure in water of 700 kPa (spatial peak pulse average intensity without ramping of 16 W/cm^2) and a focal distance of 43 mm. The measured -3 dBfocal size in water was 5 mm (lateral) by 30 mm (axial). Ramped pulses (1 ms Tukey ramp, 3.25 ms total pulse duration) were applied at a pulse repetition frequency (PRF) of 250 Hz, with a pulse train duration of 300 ms and an effective duty cycle of 50%. Of the 14 participants, 7 could not hear the stimulation at all, while the rest were either uncertain or heard it faintly. EEG was recorded from 16 channels (Fig. 1a), at 600 Hz, using the g.USBamp amplifier (g.tec medical engineering GmbH).

Participants were positioned in a chin rest. The transducer, connected to an articulated arm, was manually positioned 2 cm to the left of the inion and held in place using rubber straps. Acoustic coupling was achieved using a gel pad and ultrasound gel. Participants were dark adapted for 2 min before starting stimulation and then sat facing a screen 50–60 cm away. First, in two TUS-only blocks, real and sham pulses (100 each), were applied randomly at a fixed inter-stimulus interval of 2 s. Then, two TUS + checkerboard blocks were performed, where a checkerboard stimulus (checks at 25 and 75% of maximum screen luminance, and ~32° visual angle) was flipped every 0.5 s, and every fourth


stimulus was associated with either a real or sham (100 each) TUS trial. The TUS trial started 130 ms ($\pm 0-5$ ms jitter) before the checkerboard flip. Real and sham trials within each block were randomised and double-blind.


EEG data were analysed using eeglab (https://eeglab.org/) and FieldTrip (http://fieldtriptoolbox.org). The data were epoched relative to the TUS onset (-0.5 to 0.5 s) for TUS-only blocks, and relative to the checkerboard flip (-0.2 to 0.3 s) for TUS + checkerboard blocks. The following filters were applied: 50 Hz bandstop, 45 Hz lowpass and 1 Hz highpass, and the data were baseline corrected (-100 to 0 ms TUS-only, and -200 to -140 TUS + checkerboard). Across participants and conditions 14 ± 7 trials were rejected using z-value based artifact detection with a cut-off of 15. After time-locked averaging, cluster-based permutation testing was used to examine differences between pairs of conditions across all channels.

In the TUS-only blocks, we did not observe any evoked potentials, and found no significant differences between real and sham TUS conditions (Fig. 1b). In contrast to previous reports, none of our participants reported phosphenes. As would be expected, in the TUS + checkerboard blocks, a clear VEP in response to the visual checkerboard was observed in all conditions. A statistically significant difference was observed between real and no TUS trials, in posterior electrodes, during a time period corresponding to the N75 component of the VEP, which likely originates in V1 (Fig. 1c). There was no difference between the sham and no TUS condition, but also no significant difference when the real and sham conditions were directly compared.

Our findings differ from previous work which showed that TUS applied to the V1 evokes a 'VEP-like' potential [1]. While we used the same intensity as this previous study, in order to implement effective ramping, we lowered the PRF. Though some *in vitro* and animal data suggest that higher PRFs lead to stronger effects [6,7], the parameter space has not been extensively mapped, and in humans neuromodulatory effects have been demonstrated at PRFs similar to ours [8]. As such, while the differences in parameters may have contributed to the lack of TUS-evoked activity in our study, we cannot rule out the possibility that effects reported previously were influenced by an auditory confound, in particular since the limited number of EEG channels did not allow localizing the anatomical origin of the evoked potential.

Adding to previous work showing modulatory TUS effects [2], we observed increased amplitude of the VEP N75 component. Modulation of the N75 amplitude has also been reported in response to transcranial magnetic and electrical stimulation [9], and can be accompanied by a change in contrast sensitivity [10]. Our data

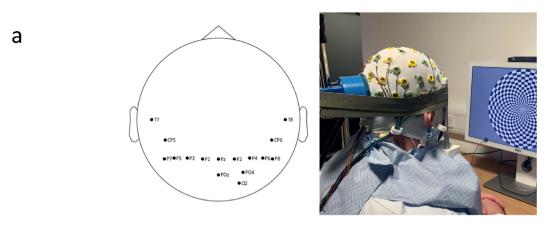

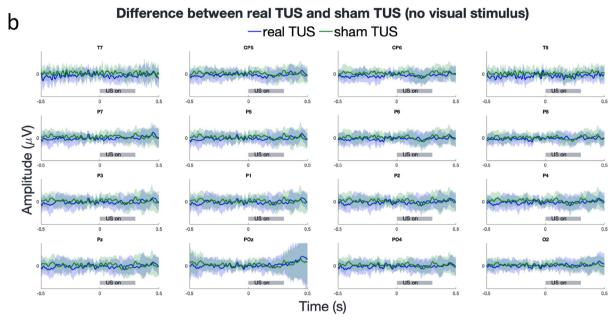

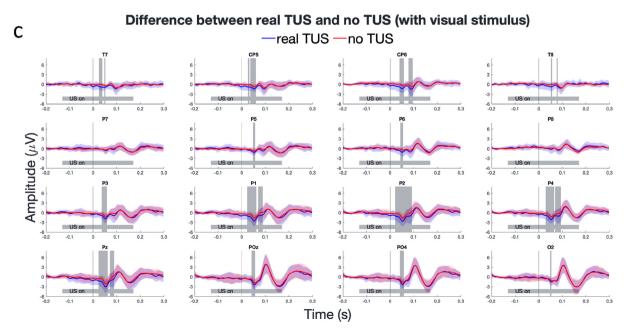


Fig. 1. Depiction of recorded EEG channels and experimental set-up (a). EEG recordings in TUS only blocks (b), and TUS + checkerboard blocks (c) where vertical grey line represents checkerboard flip. No significant differences were found between sham TUS and no TUS in TUSonly blocks. Shaded grey areas in 'c' represent the windows in which significant differences were found between real TUS and no TUS conditions.

suggest that TUS can be added to the repertoire of non-invasive brain stimulation tools to study the physiological basis of visual perception, and more generally, to modulate neural activity for basic science and clinical applications. However, we did not find any differences between sham and real TUS conditions, likely due to fewer trials in these conditions compared to the no TUS VEPs (100 vs 300), but replication studies are required to draw definitive conclusions.

In conclusion, we demonstrate that ramped TUS, which is less audible than pulsing regimes with sharp onsets and offsets, can modulate neural activity. This suggests that, in line with in-vitro and animal data, there is a direct neuromodulatory effect of ultrasound, in addition to any confounding effects. Moving forward, ramping offers a relatively easy approach to minimise the auditory confound.

Data sharing

Raw EEG data has been uploaded to https://osf.io/rbcfy/

Declaration of competing interest

The authors declare that they have no known competing financial interests or personal relationships that could have appeared to influence the work reported in this paper.

Acknowledgements

This work was supported by the Engineering and Physical Sciences Research Council UK (EP/P008860/1, EP/P008712/1, EP/S026371/1). EM was supported by a UKRI Future Leaders Fellowship (MR/T019166/1) and in part by the Wellcome/EPSRC Centre for Interventional and Surgical Sciences (WEISS) (203145Z/16/Z). CZ is supported by the Brain Research UK (201718-13). SB was supported by the Dunhill Medical Trust, (RPGF1810\93). TN was supported by a grant from the Boehringer Ingelheim Foundation (BIS) to TOB. The research was supported by the National Institute for Health Research (NIHR) Oxford Biomedical Research Centre and the NIHR Oxford Health Biomedical Research Centre. The Wellcome Centre for Integrative Neuroimaging is supported by core funding from the Wellcome Trust (203139/Z/16/Z). CJS holds a Senior Research Fellowship, funded by the Wellcome Trust (224430/Z/21/Z).

References

- [1] Lee W, Kim HC, Jung Y, Chung YA, Song IU, Lee JH, et al. Transcranial focused ultrasound stimulation of human primary visual cortex. Sci Rep 2016;6(1):
- [2] Legon W, Sato TF, Opitz A, Mueller J, Barbour A, Williams A, et al. Transcranial focused ultrasound modulates the activity of primary somatosensory cortex in humans. Nat Neurosci 2014;17(2):322–9.
- [3] Johnstone A, Nandi T, Martin E, Bestmann S, Stagg C, Treeby B. A range of pulses commonly used for human transcranial ultrasound stimulation are clearly audible. Brain Stimul: Basic. Trans. Clin. Res. Neuromodulation. 2021;14(5):1353-5.
- [4] Mohammadjavadi M, Ye PP, Xia A, Brown J, Popelka G, Pauly KB. Elimination of peripheral auditory pathway activation does not affect motor responses from ultrasound neuromodulation. Brain Stimul 2019;12(4):901–10.
- [5] Braun V, Blackmore J, Cleveland RO, Butler CR. Transcranial ultrasound stimulation in humans is associated with an auditory confound that can be effectively masked. Brain Stimul 2020;13(6):1527–34.
- [6] King RL, Brown JR, Newsome WT, Pauly KB. Effective parameters for ultrasound-induced in vivo neurostimulation. Ultrasound Med Biol 2013;39(2):312–31.
- [7] Manuel TJ, Kusunose J, Zhan X, Lv X, Kang E, Yang A, et al. Ultrasound neuro-modulation depends on pulse repetition frequency and can modulate inhibitory effects of TTX. Sci Rep 2020;10(1):1–10.

- [8] Liu C, Yu K, Niu X, He B. Transcranial focused ultrasound enhances sensory discrimination capability through somatosensory cortical excitation. Ultrasound Med Biol 2021;47(5):1356–66.
- [9] Vallar G, Bolognini N. Behavioural facilitation following brain stimulation: implications for neurorehabilitation. Neuropsychol Rehabil 2011;21(5):618–49.
- [10] Nakazono H, Ogata K, Takeda A, Yamada E, Kimura T, Tobimatsu S. Transcranial alternating current stimulation of α but not β frequency sharpens multiple visual functions. Brain Stimul 2020;13(2):343—52.

Tulika Nandi*

Wellcome Centre for Integrative Neuroimaging, FMRIB, Nuffield Department of Clinical Neuroscience, University of Oxford, Oxford, UK

Neuroimaging Center (NIC), Johannes Gutenberg University Medical Center, Mainz, Germany

Ainslie Johnstone

Department for Clinical and Movement Neuroscience, UCL Queen Square Institute of Neurology, University College London, London, UK

Fleanor Mai

Department of Medical Physics and Biomedical Engineering, University College London, London, UK

Wellcome/EPSRC Centre for Interventional & Surgical Sciences, University College London, London, UK

Catharina Zich

Wellcome Centre for Integrative Neuroimaging, FMRIB, Nuffield Department of Clinical Neuroscience, University of Oxford, Oxford, UK

Department for Clinical and Movement Neuroscience, UCL Queen Square Institute of Neurology, University College London, London, UK

Robert Cooper

Department of Medical Physics and Biomedical Engineering, University College London, London, UK

Sven Bestmann

Department for Clinical and Movement Neuroscience, UCL Queen Square Institute of Neurology, University College London, London, UK

Wellcome Centre for Human Neuroimaging, UCL Queen Square Institute of Neurology, University College London, London, UK

Til Ole Bergmann

Neuroimaging Center (NIC), Johannes Gutenberg University Medical Center, Mainz, Germany

Leibniz Institute for Resilience Research, Wallstraße 7-9, 55122, Mainz, Germany

Bradley Treeby

Department of Medical Physics and Biomedical Engineering, University College London, London, UK

Charlotte J. Stagg

Wellcome Centre for Integrative Neuroimaging, FMRIB, Nuffield Department of Clinical Neuroscience, University of Oxford, Oxford, UK

Medical Research Council Brain Network Dynamics Unit, University of Oxford, Oxford, UK

* Corresponding author. NeuroImaging Center (NIC), Johannes Gutenberg University Medical Center, Langenbeckstr. 1, Bldg. 308c, 55131, Mainz, Germany.

E-mail address: tulika.nandi@ndcn.ox.ac.uk (T. Nandi).

26 January 2023

Available online 6 February 2023